

OmniKine™

Human IL-1beta Colorimetric Sandwich ELISA Kit

Catalog #: OK-0227

**Detection and Quantification of Human IL-1beta
Concentrations in Supernatants, Sera and Plasma.**

**Research Purposes Only. Not Intended for Diagnostic or
Clinical Procedures.**

**Store entire kit at 4°C until use.
Kit expiration is 3 months from date of shipment**

Manual Version: 1.8.622

| CONTENTS | PAGE |
|--|-------------|
| Introduction..... | 3 |
| Assay Principles..... | 4 |
| Assay Format..... | 5 |
| Materials Included/Additional Materials Required..... | 6 |
| Sample Preparation and Storage..... | 7 |
| Reagent Preparation..... | 8 |
| Assay Procedure..... | 9 |
| Data Analysis/ Typical Data..... | 10 |
| Recovery and Linearity..... | 11 |
| Sensitivity, Cross Reactivity, Specificity..... | 12 |
| Summarized Protocol..... | 13 |
| Health and Safety Precautions/ Assay Restrictions..... | 14 |
| ELISA Plate Template..... | 15 |
| Technical Support..... | 16 |

INTRODUCTION

Produced by activated macrophages, IL-1 stimulates thymocyte proliferation by inducing IL-2 release, B-cell maturation and proliferation, and fibroblast growth factor activity. IL-1 proteins are involved in the inflammatory response, being identified as endogenous pyrogens, and are reported to stimulate the release of prostaglandin and collagenase from synovial cells. The lack of a specific hydrophobic segment in the precursor sequence suggests that IL-1 is released by damaged cells or is secreted by a mechanism differing from that used for other secretory proteins. The similarity among the IL-1 precursors suggests that the amino ends of these proteins serve some as yet undefined function. The protein encoded by IL-1b is a member of the interleukin 1 cytokine family. This cytokine is produced by activated macrophages as a proprotein, which is proteolytically processed to its active form by caspase 1 (CASP1/ICE). This cytokine is an important mediator of the inflammatory response, and is involved in a variety of cellular activities, including cell proliferation, differentiation, and apoptosis. The induction of cyclooxygenase-2 (PTGS2/COX2) by this cytokine in the central nervous system (CNS) is found to contribute to inflammatory pain hypersensitivity. IL-1b and eight other interleukin 1 family genes form a cytokine gene cluster on chromosome 2.

ASSAY PRINCIPLES

The OmniKine™ Human IL-1beta ELISA Kit contains the components necessary for quantitative determination of natural or recombinant Human IL-1beta concentrations within any experimental sample including cell lysates, serum and plasma. This particular immunoassay utilizes the quantitative technique of a “Sandwich” Enzyme-Linked Immunosorbent Assay (ELISA) where the target protein (antigen) is bound in a “sandwich” format by the primary capture antibodies coated to each well-bottom and the secondary detection antibodies added subsequently by the investigator.

The capture antibodies coated to the bottom of each well are specific for a particular epitope on Human IL-1beta while the user-added detection antibodies bind to epitopes on the captured target protein. Amid each step of the procedure, a series of wash steps must be performed to ensure the elimination of non-specific binding between proteins to other proteins or to the solid phase.

After incubation and “sandwiching” of the target antigen, a peroxidase enzyme is conjugated to the constant heavy chain of the secondary antibody (either covalently or via Avidin/Streptavidin-Biotin interactions), allowing for a colorimetric reaction to ensue upon substrate addition. When the substrate TMB (3, 3', 5, 5'-Tetramethylbenzidine) is added, the reaction catalyzed by peroxidase yields a blue color that is representative of the antigen concentration.

Upon sufficient color development, the reaction can be terminated through addition of Stop Solution (2 N Sulfuric Acid) where the color of the solution will turn yellow. The absorbance of each well can then be read by a spectrophotometer, allowing for generation of a standard curve and subsequent determination of protein concentration.

ASSAY FORMAT


Capture Antibody



Capture antibodies specific for the target are coated to the plate. Additional binding sites on the plate are blocked.


Target Antigen



Target antigen present in standard or sample is bound by capture antibodies on the solid-phase.


Biotinylated Detection Antibody



Biotinylated detection antibodies specific for the target are added to bind another epitope on the target antigen.


Streptavidin-HRP



Streptavidin-HRP attaches to detection antibody via high affinity streptavidin-biotin interaction.


Unreacted TMB


Blue TMB Diimine Product



TMB substrate is converted to the blue TMB diimine via the HRP enzyme. Upon addition of acid, the reaction terminates and the wells can be read at 450 nm.

MATERIALS INCLUDED

| Component | Quantity Per Kit | Storage/Stability after first use |
|--|-------------------------|-----------------------------------|
| Microstrips Coated w/ Capture Antibody | 12 x 8-Well Microstrips | 1 month at 4°C |
| Protein Standard | Lyophilized | |
| Biotinylated Detection Antibody | Lyophilized | |
| 400x Streptavidin-HRP B | 30 µl | |
| Wash Buffer (15x) | 50 ml | |
| Assay Diluent 10WR | 15 ml | |
| Assay Diluent 1TD | 50 ml | |
| Ready-to-Use Substrate | 12 ml | |
| Stop Solution | 12 ml | |
| Adhesive Plate Sealers | 2 Sheets | |
| Technical Manual | 1 Manual | - |

Any unused strips should be rewrapped with plate sealer and placed back into pouch with zipper closed until next use**

ADDITIONAL MATERIALS REQUIRED

The following materials and/or equipment are NOT provided in this kit but are necessary to successfully conduct the experiment:

- Microplate reader able to measure absorbance at 450 nm (with correction wavelength set to 540 nm or 570 nm)
- Micropipettes ranging from 1 µl to 1 ml
- Distilled, deionized, and or purified water (recommended TOC 1-50 ppb, MΩ-cm 18.0)
- Squirt bottle, manifold dispenser, multichannel pipette reservoir or automated microplate washer
- Graph paper or computer software capable of generating or displaying logarithmic functions
- Absorbent paper or vacuum aspirator
- Test tubes or microfuge tubes capable of storing ≥1 ml
- Bench-top centrifuge (optional)
- Bench-top vortex (optional)
- Orbital shaker (optional)

SAMPLE PREPARATION AND STORAGE

| Sample Type | Recommended Dilution Factor |
|--------------------------|-----------------------------|
| Plasma | 1 to 10 |
| Serum | 1 to 10 |
| Cell Culture Supernatant | 1 to 5 |

Levels of Human IL-1beta may vary between samples. Optimal dilution factors for every sample must be determined by the investigator.

Cell Supernatants

Remove large cell components via centrifugation and perform the assay. Dilute cell supernatants at a minimum of 1 to 5 using Assay Diluent 1TD and assay.

Serum

Allow samples to clot in a serum separator tube (SST) for 30 minutes. After sufficient clotting, centrifuge at 1000 x g for 15 minutes and remove serum from SST in preparation for the assay. Dilute serum samples 1 to 10 using Assay Diluent 10WR and incubate 20 mins room temperature (RT) prior to continuing with the assay

Plasma

Use heparin, citrate or EDTA as an anticoagulant to gather plasma from original biological sample. After collection of the plasma, centrifuge for 15 minutes at 1000 x g. This step must be performed within 30 minutes of plasma collection. Dilute plasma samples 1 to 10 using Assay Diluent 10WR and incubate 20 mins prior to RT prior to continuing with the assay.

If samples are to be used within 24 hours, aliquot and store at 4°C. If samples are to be used over a long period of time, aliquot and store between -20°C and -80°C, depending on the duration of storage.

Samples containing a visible precipitate or pellet must be clarified prior to use in the assay.

Avoid repeated freeze/thaw cycles to prevent loss of biological activity of proteins in experimental samples.

REAGENT PREPARATION

All provided solutions should be at ambient temperature prior to use. **We recommend performing the assay in duplicate.** Reagents provided are enough to assay 96 wells and it is recommended to only prepare as much needed on the day of the experiment. All incubation steps should be performed on an orbital shaker to equilibrate solutions when added to the microplate wells.

1. Dilute the 15x Wash Buffer to 1x Wash Buffer using 14 volumes of ddH₂O and 1 volume of 15x Wash Buffer.
2. Reconstitute Detection Antibody with 100 µl of ddH₂O for a concentration of 100x. Mix gently and dilute to 1x prior to use.
3. Reconstitute Protein Standard with 83 µl of ddH₂O for a concentration of 75ng/ml. Mix gently and dilute to the working range of the kit, 4-250 pg/ml pg/mL. To obtain a 7 point 2 fold dilution for the standard curve 2.33 µl of standard into 697.66 µl of diluent.
 - a. Dilute Protein Standard with Assay Diluent 10WR when experimenting with Serum/Plasma samples. **OR.**
 - b. Dilute Protein Standard with Assay Diluent 1TD when experimenting with Cell Supernatant samples.



4. Mix the 400x Streptavidin-HRP B (SAV-HRP) gently. Dilute to 1x using Assay Diluent 1TD.
5. Stop Solution and Ready to Use Substrate are ready to use and do not need dilution.

ASSAY PROCEDURE

1. Prepare all reagents to working concentrations, standards to desired range, and samples to appropriate dilution factors.
2. Remove desired number of capture antibody coated strips for experiment and place remaining strips back into dry pouch with desiccant for 4°C storage.
3. Add 100 µl of Standards/ Samples to each well and incubate on orbital shaker at room temperature (RT) for 2 hrs.
4. Aspirate the solution and add 300 µl of 1x Wash Buffer to each well being used and gently shake for 2-3 mins on an orbital shaker. Repeat this process 3 times. After the last wash ensure no liquid remains by inverting the plate and tapping it against clean paper towels.
5. Add 100 µl of 1x Detection Antibody to each well and incubate for 2 hrs. on an orbital shaker at RT.
6. Repeat step 4.
7. Add 100 µl of 1x SAV-HRP B to each well and incubate for 30 mins on an orbital shaker at RT
8. Repeat step 4.
9. Add 100 µl of Ready to use Substrate to each well, cover plate from light, and incubate for 15 mins on an orbital shaker at RT.
10. Add 100 µl of Stop Solution to each well and read at 450 nm.


DATA ANALYSIS

Average the duplicate or triplicate readings for each standard, control and sample and subtract the average zero standard optical density.

Generate a standard curve by using Microsoft Excel or other computer software capable of establishing a 4-Parameter Logistic (4-PL) curve fit. If using Excel or an alternative graphing tool, plot the average optical density values in absorbance units (y-axis) against the known standard concentrations in pg/ml (x-axis).

Only use the values in which a noticeable gradient can be established. Afterwards, generate a best fit curve or “trend-line” through the plotted points via regression analysis.

TYPICAL DATA

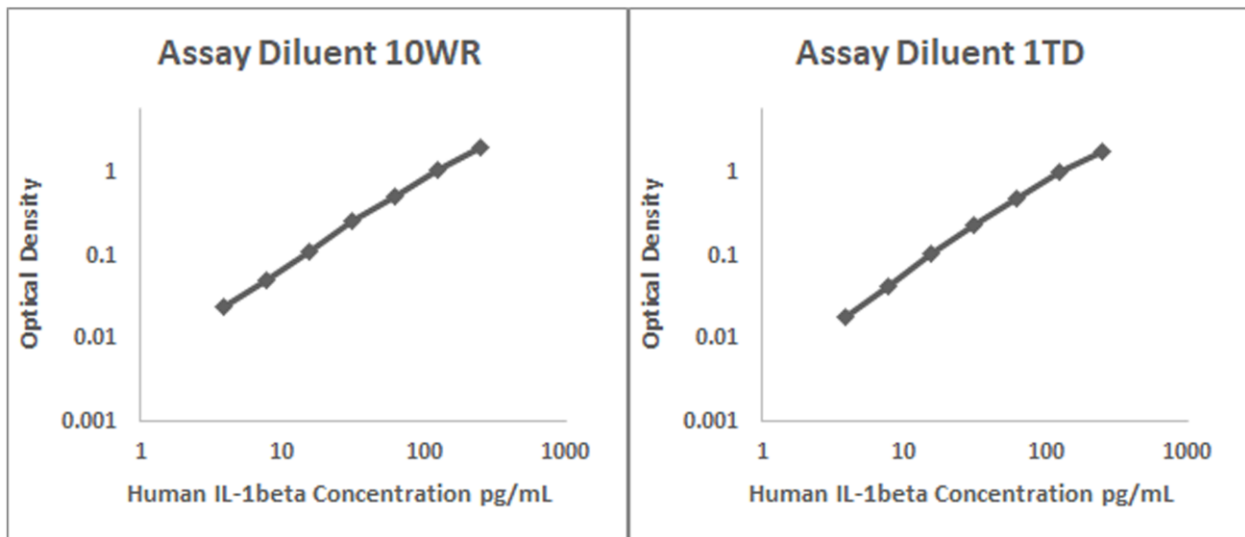

| | | | | | | | |
|---|--------|--------|-------|-------|-------|------|------|
| Concentration pg/ml | 250.00 | 125.00 | 62.50 | 31.25 | 15.63 | 7.81 | 3.91 |
| Average Optical Density 10WR | 2.06 | 1.10 | 0.52 | 0.26 | 0.11 | 0.05 | 0.03 |
| Average Optical Density 1TD | 1.87 | 1.01 | 0.51 | 0.23 | 0.11 | 0.04 | 0.02 |

The data and subsequent graph were obtained after performing a cytokine ELISA for Human IL-1beta. Each known sample concentration was assayed in triplicate.

The standard curves shown are for demonstration. A new curve must be generated for each experiment.

RECOVERY

Three concentrations of recombinant Human IL-1beta was spiked into various samples to measure the recovery percentage of recombinant protein in duplicate.

| Sample Type | Average Recovery % | Range % |
|--------------------|--------------------|---------|
| Plasma (10%) | 90 | 86-95 |
| Serum (10%) | 97 | 95-101 |
| RPMI 10% FBS (20%) | 113 | 103-119 |

LINEARITY

Human IL-1beta recombinant protein was spiked into various biological samples and serial diluted with Assay Diluent 10WR for serum samples and Assay Diluent 1TD for RPMI 10% FBS.

| | | EDTA Plasma | Serum | RPMI 10% FBS |
|--------|------------|-------------|-------|--------------|
| Neat | pg/ml | 59.10 | 63.16 | 129.85 |
| | Expected % | 95 | 101 | 104 |
| 1 to 2 | pg/ml | 28.66 | 30.86 | 36.15 |
| | Expected % | 99 | 92 | 116 |
| 1 to 4 | pg/ml | 13.65 | 12.45 | 18.70 |
| | Expected % | 80 | 80 | 119 |
| 1 to 8 | pg/ml | 7.55 | 7.66 | 8.49 |
| | Expected % | 98 | 98 | 109 |

SENSITIVITY

The Human IL-1beta ELISA Kit allows for the detection and quantification of endogenous levels of natural and/or recombinant Human IL-1beta proteins within the range of 4-250 pg/ml pg/ml.

CROSS REACTIVITY AND SPECIFICITY

The OmniKine™ Human IL-1beta ELISA is capable of recognizing both recombinant and naturally produced Human IL-1beta proteins. The antigens listed below were tested at 50 ng/ml and did not exhibit significant cross reactivity or interference.

- Human: IL-1alpha
- Murine: IL-1alpha, IL-1beta
- Rat: IL-1alpha

SUMMARIZED PROTOCOL

Reconstitute Biotinylated Detection Antibody and Protein Standard and dilute the 15x Wash Buffer as specified.



Perform serial dilution of Protein Standard and prepare samples as desired. See sample preparation section for instructions to dilute serum and plasma samples.



Add 100ul of Protein Standard, sample or control to each well and incubate for 2 hours at room temperature.



Aspirate Protein Standards, samples or controls out and wash plate 4 times.



Dilute Biotinylated Detection Antibody as specified. Add 100ul to each well and incubate for 2 hours at room temperature.



Aspirate Biotinylated Detection Antibody out and wash plate 4 times.



Dilute 400x Streptavidin-HRP as specified. Add 100ul of 1x Streptavidin-HRP to each well and incubate at room temperature for 30 minutes.



Aspirate 1x Streptavidin-HRP out and wash plate 4 times.



Add 100ul of Ready-to-Use Substrate to each well and incubate at room temperature for color development.



Add 100ul of Stop Solution and read plate at 450nm.


HEALTH AND SAFETY PRECAUTIONS

- Reagents provided in this kit may be harmful if ingested, inhaled or absorbed through the skin. Please carefully review the MSDS for each reagent before conducting the experiment.
- Stop Solution contains 2 N Sulfuric Acid (H_2SO_4) and is an extremely corrosive agent. Please wear proper eye, hand and face protection when handling this material. When the experiment is finished, be sure to rinse the plate with copious amounts of running water to dilute the Stop Solution prior to disposing the plate.

ASSAY RESTRICTIONS

- This ELISA kit is intended for research purposes only, NOT diagnostic or clinical procedures of any kind.
- Materials included in this kit should NOT be used past the expiration date on the kit label.
- Reagents or substrates included in this kit should NOT be mixed or substituted with reagents or substrates from any other kits.
- Variations in pipetting technique, washing technique, operator laboratory technique, kit age, incubation time or temperature may cause differences in binding affinity of the materials provided.
- The assay is designed to eliminate interference and background by other cellular macromolecules or factors present within any biological samples. However, the possibility of background noise cannot be fully excluded until all factors have been tested using the assay kit.
- Individual results may vary due to differences in technique, plasticware and water sources.

ELISA PLATE TEMPLATE

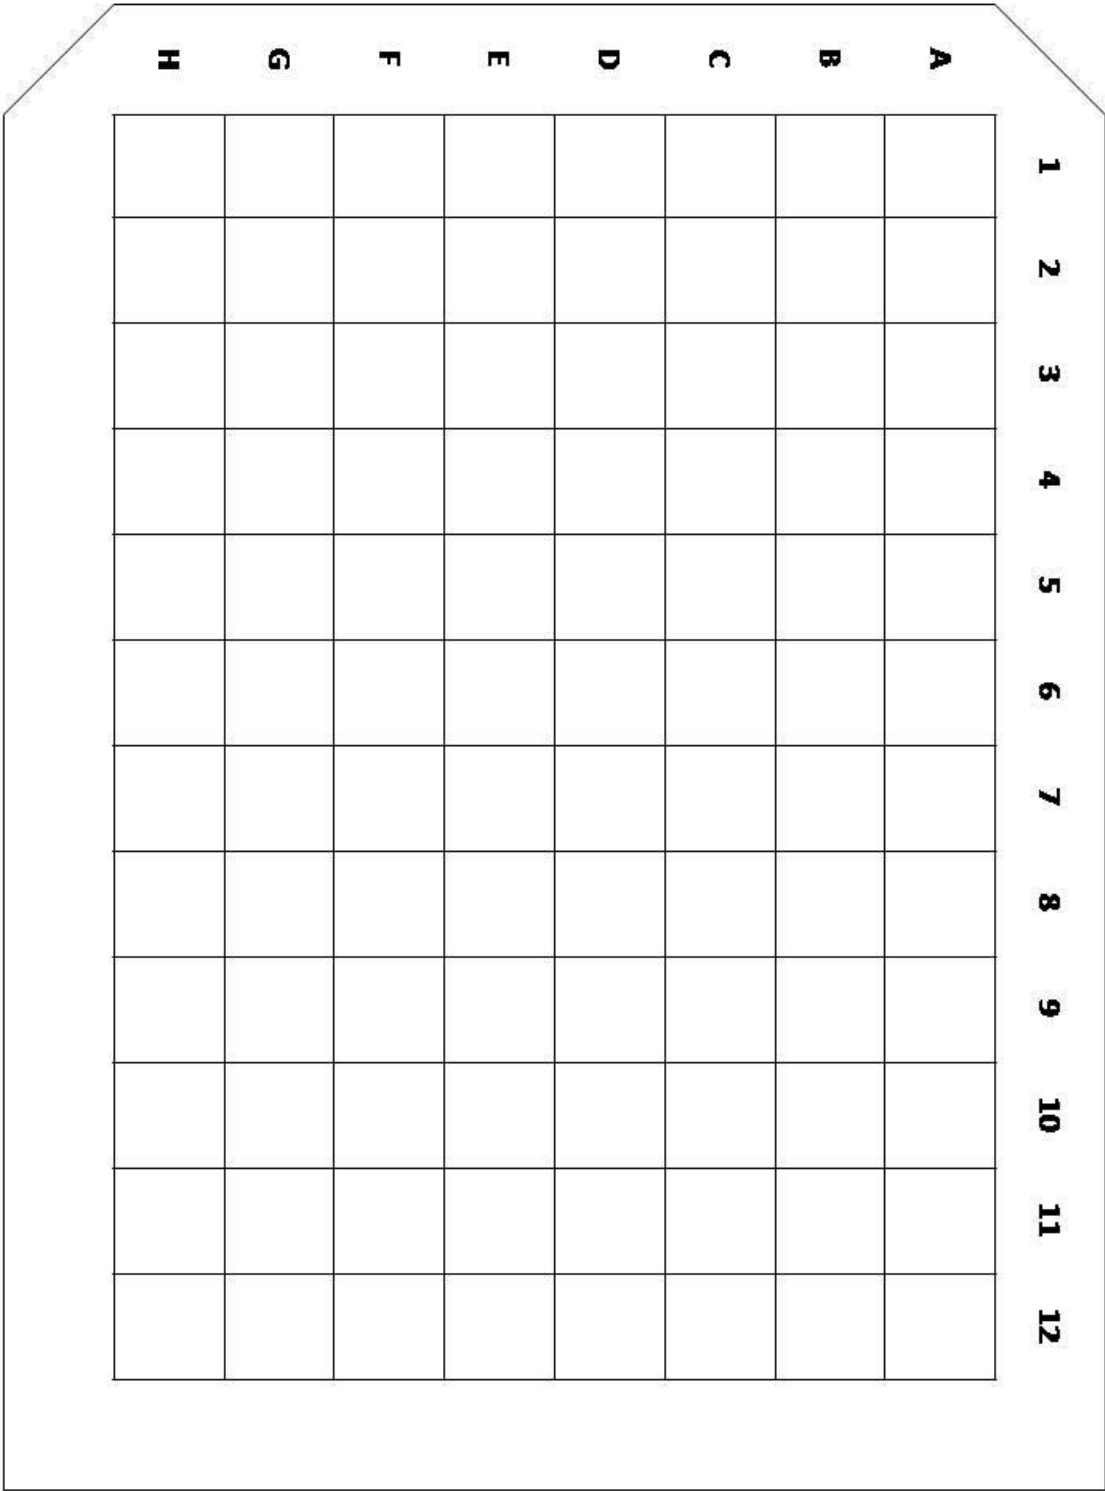

The image shows a template for an ELISA plate. It consists of a grid of 96 wells arranged in 8 columns and 12 rows. The columns are labeled A through H from left to right, and the rows are labeled 1 through 12 from top to bottom. The top-left corner of the plate is cut off at a 45-degree angle. The grid is empty, with no data or text inside the wells.

| | A | B | C | D | E | F | G | H |
|----|---|---|---|---|---|---|---|---|
| 1 | | | | | | | | |
| 2 | | | | | | | | |
| 3 | | | | | | | | |
| 4 | | | | | | | | |
| 5 | | | | | | | | |
| 6 | | | | | | | | |
| 7 | | | | | | | | |
| 8 | | | | | | | | |
| 9 | | | | | | | | |
| 10 | | | | | | | | |
| 11 | | | | | | | | |
| 12 | | | | | | | | |

TECHNICAL SUPPORT

For troubleshooting, information or assistance, please go online to www.assaybiotech.com or contact us at:

Assay Biotechnology Company, Inc.
47787 Fremont Blvd.
Fremont, CA 94538
United States of America

Email: tech@assaybiotech.com

Phone: (408) 747-0185
Toll-Free Phone: (877) 883-7988

Fax: (408) 747-0145
Toll-Free Fax: (877) 610-9758



**Over 2,000 Assay Kits including Sandwich, Cell-Based and
Transcription Factor ELISA Kits**

Visit us at www.assaybiotech.com